



User Manual – RC-18/19

Single-Use Temperature Logger

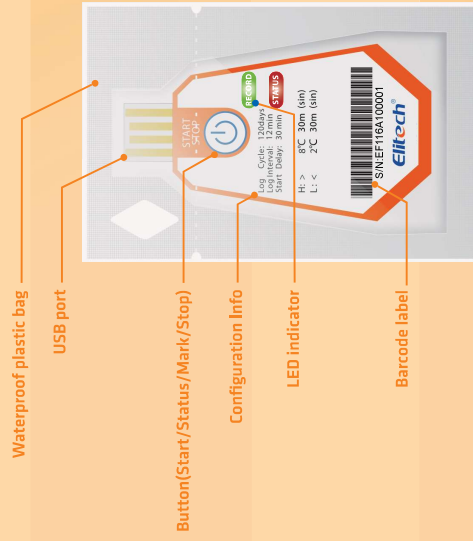

Frontside

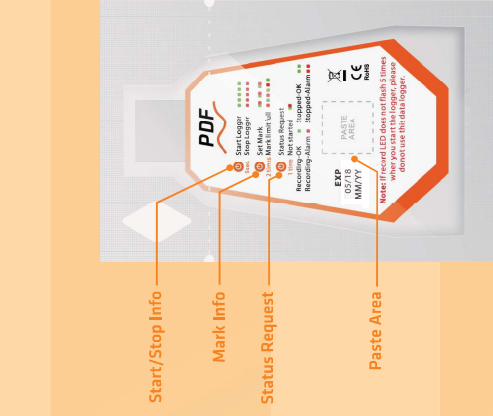

Backside

Note: The picture is for reference only. Any discrepancy in future, please adhere to the final product.

Operation Instructions




01 Keep button pressed for minimum 5 seconds to start recording. Then RECORD LED flashes 5 times, which indicates a successful starting. If STATUS LED is lit for 3 seconds, please do not use the logger(indicating low battery)! Tear off serial number label for your reference.



02 Press button once at any time to check current status of the logger. Double-click button to set a mark in the report. See details of these optional features in tables below.



03 Keep button pressed for minimum 5 seconds to stop recording. Then STATUS LED flashes 5 times, which indicates a successful stopping.



04 After stopping record, tear off the transparent plastic cover and connect the logger to a USB port of the computer. The PDF and report will be generated automatically and can be found in the device's folder.

Product Overview

This document describes specific validation procedures for RC-18/19 data loggers, for the purpose to ensure the proper operation and provide a reliable temperature and time record during transportation and storage.

Technical Specifications

Recording Options	Single-Use
Temperature Range	-30 °C to 70 °C
Temperature Accuracy	±0.5 (-20°C/+40°C); ±1.0 (other range)
Temperature Resolution	0.1 °C
Data Storage Capacity	16,000 readings
Shelf Life / Battery	2 years ¹ / CR2450 button cell
Recording Interval	6 minutes (standard, others on request)
Recording Duration	up to 180 days ² (standard, others on request)
Startup Mode	Button or software
Stop Mode	Button, software or stop when full
Protection Class	IP67 / NEMA 6
Dimensions	80mm x 48mm x 5.8mm (L x W x H)
Weight	Approx. 15g

Certifications	EN 12830, CE, RoHS
Validation Certificate	Hardcopy and PDF file in memory
Software	ElitechLog Win (V1.0.0 or newer) ElitechLog Mac (V1.0.0 or newer)
Report Generation	Automatic PDF
Password Protection	Optional on request
Connection Interface	USB 2.0, A-Type
Alarm Configuration	Optional, up to 5 points
Reprogrammable	ElitechLog Win (V1.0.0 or newer) ElitechLog Mac (V1.0.0 or newer)
Accessories incl.	Shipping Documents, Certificate, Reprogram Label and Seal-Bag
1	Depending on optimal storage conditions (+15 °C to +23 °C / 45% to 75% RH)
2	Depending on application temperature (very low / high temperatures may shorten it)

Operation Indication

Start / Stop

Status	Action	LED confirmation
Start Logger	5 sec pushing button	RECORD LED flashing 5 times ●●●●●
Set Mark	double-click button	STATUS LED + RECORD LED flashing 5 times ●●●●●●●
Stop Logger	5 sec pushing button	STATUS LED flashing 5 times ●●●●●

Status Request by pushing Button 1 time

Status	Action	LED confirmation
Not Started	push button 1 time	STATUS LED + RECORD LED flashing 1 time ●●
Recording - OK	push button 1 time	RECORD LED flashing 1 time ●
Recording - Alarm	push button 1 time	STATUS LED flashing 1 time ●●
Stopped - OK	push button 1 time	RECORD LED flashing 2 times ●●
Stopped - Alarm	push button 1 time	STATUS LED flashing 2 times ●●●